General Warranty

We warrant that the product will be free from defects in materials and workmanship for a period of 3 years from the date of purchase of the product by the original purchaser from our company. The warranty period for accessories such as probes, battery is 12 months. This warranty only applies to the original purchaser and is not transferable to a third party.

If the product proves defective during the warranty period, we will either repair the defective product without charge for parts and labour, or will provide a replacement in exchange for the defective product. Parts, modules and replacement products used by our company for warranty work may be new or reconditioned like new. All replaced parts, modules and products become the property of our company.

In order to obtain service under this warranty, the customer must notify our company of the defect before the expiration of the warranty period. Customer shall be responsible for packaging and shipping the defective product to the designated service centre, a copy of the customers proof of purchase is also required.

This warranty shall not apply to any defect, failure or damage caused by improper use or improper or inadequate maintenance and care. We shall not be obligated to furnish service under this warranty a) to repair damage resulting from attempts by personnel other than our company representatives to install, repair or service the product; b) to repair damage resulting from improper use or connection to incompatible equipment; c) to repair any damage or malfunction caused by the use of not our supplies; or d) to service a product that has been modified or integrated with other products when the effect of such modification or integration increases the time or difficulty of servicing the product.

Please contact the nearest Sales and Service Offices for services.

Excepting the after-sales services provided in this summary or the applicable warranty statements, we will not offer any guarantee for maintenance definitely declared or hinted, including but not limited to the implied guarantee for marketability and special-purpose acceptability. We should not take any responsibilities for any indirect, special or consequent damages.

※：The illustrations, interface, icons and characters in the user manual may be slightly different from the actual product. Please refer to the actual product.

Table of Contents

1. General Safety Requirement 1

2. Safety Terms and Symbols 2

3. General Inspection 3

4. Quick Start 4

Front panel overview 4
Rear Panel Overview 5
Power on 6
User Interface 6
Set the channel 7
Set basic waveform 8
Output the built-in waveform (including DC) 9
Generate the Modulated Waveform 10
Generate Sweep 11
Generate Burst 11
Store 11
Reading waveform 11
Write and Recall waveform 12
Utility Setting 14
Counter 14

5. Communication with PC 16

6. Appendix 17

Appendix A：Accessories 17
Appendix B：General Care and Cleaning 17

1. General Safety Requirement

Before any operations, please read the following safety precautions to avoid any possible bodily injury and prevent this product or any other products connected from damage. In order to avoid any contingent danger, this product is only used within the range specified.

Use Proper Power Cord. Use only the power cord supplied with the product and certified to use in your country.

Product Grounded. This instrument is grounded through the power cord grounding conductor. To avoid electric shock, the grounding conductor must be grounded. The product must be grounded properly before any connection with its input or output terminal.

Limit operation to the specified measurement category, voltage, or amperage ratings.

Check all Terminal Ratings. To avoid instrument damage and the risk of electric shock, check all the Measurement Limits and markers of this product. Refer to the user's manual for the Measurement Limits before connecting to the instrument. Do not exceed any of the Measurement Limits defined in the following section.

Do not operate without covers. Do not operate the instrument with covers or panels removed.

Use Proper Fuse. Use only the specified type and rating fuse for this instrument.

Avoid exposed circuit. Do not touch exposed junctions and components when the instrument is powered.

Do not operate if in any doubt. If you suspect damage occurs to the instrument, have it inspected by qualified service personnel before further operations.

Use your instrument in a well-ventilated area. Inadequate ventilation may cause increasing of temperature or damages to the device. Please keep well ventilated and inspect the intake regularly.

Do not operate in wet conditions. In order to avoid short circuiting to the interior of the device or electric shock, please do not operate in a humid environment.

Do not operate in an explosive atmosphere.

Keep product surfaces clean and dry.

BNC output ports not allowed to input any signal such as voltage, current and other electrical signal, otherwise, it will be burned.

2. Safety Terms and Symbols

Terms in this Manual. The following terms may appear in this manual:

Warning: Warning indicates the conditions or practices that could result in injury or loss of life.

Caution: Caution indicates the conditions or practices that could result in damage to this product or other property.

Terms on the Product. The following terms may appear on this product:

Danger: It indicates an injury or hazard may immediately happen.

Warning: It indicates an injury or hazard may be accessible potentially.

Caution: It indicates a potential damage to the instrument or other property might occur.

Safety Symbols

Symbols on the Product. The following symbol may appear on the product:


Hazardous Voltage


Refer to Manual


Protective Earth Terminal


Chassis Ground


Test Ground

3. General Inspection

After you get a new generator, it is recommended that you should make a check on the instrument according to the following steps:

1. Check whether there is any damage caused by transportation.

If it is found that the packaging carton or the foamed plastic protection cushion has suffered serious damage, do not throw it away first till the complete device and its accessories succeed in the electrical and mechanical property tests.

2. Check the Accessories

The supplied accessories have been already described in *Appendix*

Appendix A：Accessories of this manual. You can check whether there is any loss of accessories with reference to this description. If it is found that there is any accessory lost or damaged, please get in touch with our distributor responsible for this service or our local offices.

3. Check the Complete Instrument

If it is found that there is damage to the appearance of the instrument, or the instrument can not work normally, or fails in the performance test, please get in touch with our distributor responsible for this business or our local offices. If there is damage to the instrument caused by the transportation, please keep the package. With the transportation department or our distributor responsible for this business informed about it, a repairing or replacement of the instrument will be arranged by us.

4. Quick Start

Front panel overview

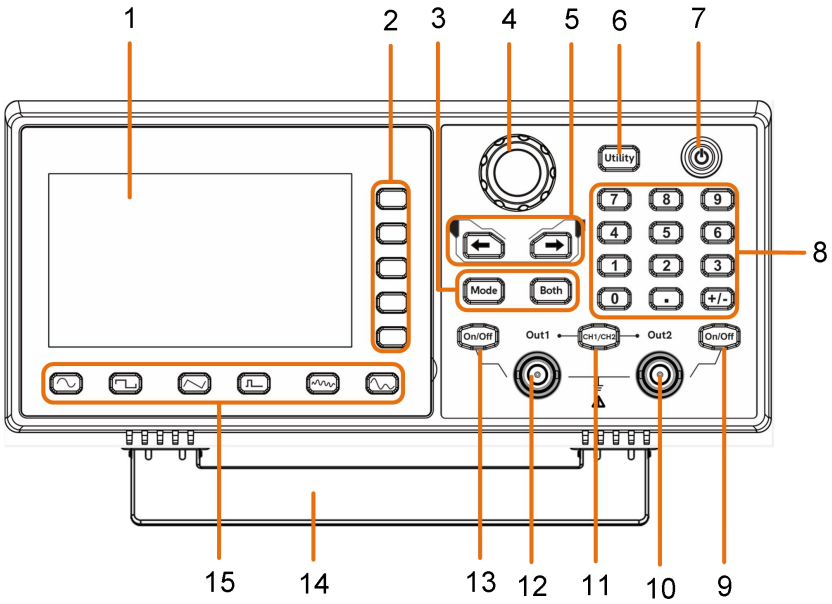


Figure 4- 1 Front Panel overview

1	**LCD**	Display the user interface.
2	**Menu selection keys**	Includes 5 keys to activate the corresponding menu.
3	**Operation keys**	**Mode:**Output the modulated waveform. **Both:**Display the editable parameters of both channels.
4	**Knob**	Change the currently selected value, also used to select the arbitrary waveform types and arbitrary data file name. When in the sweep or burst manual modes, press this knob to trigger manually.
5	**Direction key**	Move the cursor of the selected parameter.
6	**Operation key(Utility)**	Set the utility function.
7	**Power button**	Turn on/off the waveform generator.
8	**Number keypad**	Input the parameter.
9	**On/Off button**	Turns the output of the CH2 channel on or off. When the output is turned on, the backlight of the button lights up.

10	**Out 2**	Output CH2 signal.
11	**CH1/CH2**	Switch channel displayed on the screen between CH1 and CH2.
12	**Out 1**	Output CH1 signal.
13	**On/Off button**	Turns the output of the CH1 channel on or off. When the output is turned on, the backlight of the button lights up.
14	**Foot Stool**	Tilt the signal generator for easy operation.
15	**Waveform Selection area**	Includes: Sine, Square, Ramp, Pulse, Noise, Arb Wave.

Rear Panel Overview

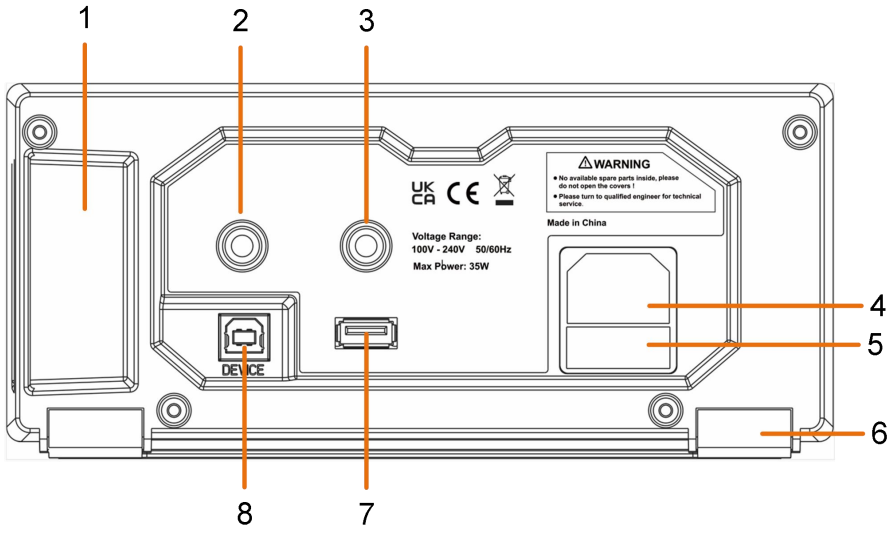


Figure 4- 2 Rear Panel Overview

1	**Handle**	
2	**Signal connector**	Used to connect the input or output of a functional signal.
3	**Counter input**	Used to receive the frequency meter input signal.
4	**AC input connector**	AC input connector.
5	**Fuse Container**	The place to install the fuse.
6	**Foot Stool**	Tilt the signal generator for easy operation.

7	**USB interface**	Connect with external USB devices, e.g. USB stick.
8	**USB Device interface**	Used to connect a USB type B controller. Can be connected with PC, the signal generator can be controlled by the host computer software.

Power on

(1) Connect the instrument to an AC power source using the power cord supplied with the accessory.

> **Warning:**
> To prevent electric shock, make sure the instrument is properly grounded.

(2) Press the **power button** on the front panel. The back of the power channel switch will light up, and the buzzer will sound.

User Interface

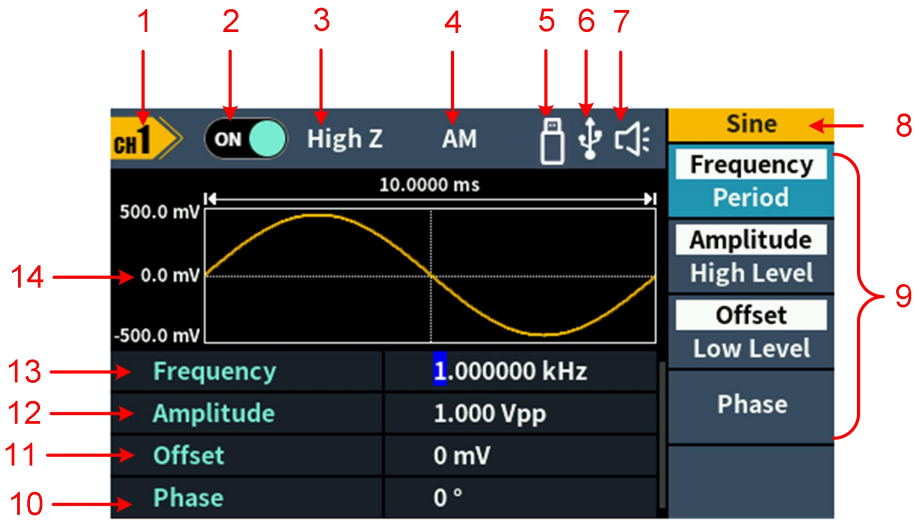


Figure 4- 3 User Interface

1	Display channel name.
2	Display channel switch status.
3	Display load.
4	Current modulation mode.
5	When the instrument detects the USB flash drive, it lights up the indicator.
6	Lights up the indicator when connected to the USB Host via the USB DEVICE interface.

7	Buzzer.
8	Menu title.
9	Current waveform or mode setting menu.
10	Start phase.
11	Offset/Low level,depending on the right highlighted menu item.
12	Amplitude/High level,depending on the right highlighted menu item.
13	Frequency/Period, depending on the highlighted menu item on the right.
14	Display current waveform.

Set the channel

- **Select the channel for configuration**

Before configuring waveform parameters, you must first select the channel you want to configure. Press **CH1/CH2** to switch to the desired channel, and the user interface displays channel information.

- **To Display/Edit Both Channels**


Press **Both** button to display the parameters of both channels.

To switch channel: Press **CH1/CH2** to switch the editable channel.

To select waveform: Press , to select waveform of current channel.

To select parameter: Press **Menu selection keys** to choose the **Parameter 1** to **Parameter 4(Corresponding keys 2-5);** Press it again to switch the current parameter such as Frequency/Period.

To edit parameter: Turn the **knob** to change the value of cursor position. Press  direction key to move the cursor. (The number keys can not be used to input.)

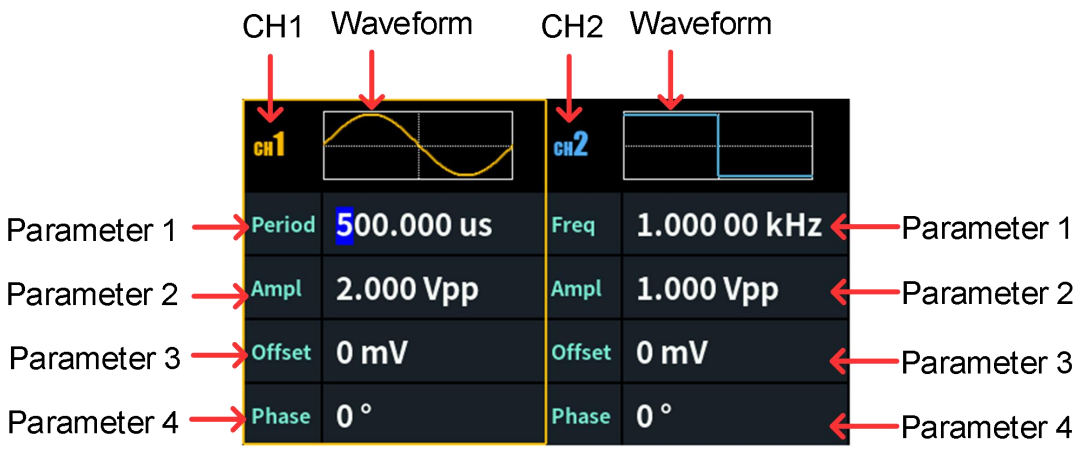

- **Turn on/off channel output**

Press CH1 **On/Off** or CH2 **On/Off** on the front panel to turn on/off the corresponding channel output. The channel will light up when it is set to output.

Set basic waveform

Can set and output the Sine, Square, Ramp, Pulse, Noise or Arbitrary waveform. Press the waveform selection button on the front panel of the instrument: sine, square, ramp, pulse, noise, arbitrary, and enter the corresponding waveform setting interface. The waveform is different and the parameters that can be set are different.

Example: Press the key and press the **Frequency/Period** softkey. The selected menu item is highlighted on white, and the cursor will display on corresponding parameter item in the user interface. Press the **Frequency/Period** softkey to switch the frequency/period.

There are two ways to change the selected parameter value:

- Turn the **knob** to increase or decrease the value at the cursor. Press the direction keys to move the cursor left or right.
- Press a **number keypad** on the numeric keypad directly, the screen will pop out of the data input box, continue to input the desired value.Press the right menu softkey to select the unit of the parameter. Press the **Back** softkey to cancel the current entry.



Figure 4-4：Use numeric keypad to set the frequency

Parameters of waveforms

Waveform	Menu Items
Sine	Frequency/Period, Amplitude/High Level, Offset/Low Level, Phase
Square	Frequency/Period, Amplitude/High Level, Offset/Low Level, Phase
Ramp	Frequency/Period, Amplitude/High Level, Offset/Low Level, Phase,Symmetry
Pulse	Frequency/Period, Amplitude/ High Level, Offset/Low Level, Phase, Width/Duty, Rise,Fall
Noise	Amplitude/High Level, Offset/Low Level
Arbitrary	Frequency/Period, Amplitude/High Level, Offset/Low Level, Phase, Built-in,Store

Output the built-in waveform (including DC)

(1) Press the button, then press the **NextPage** softkey to enter the NextPage menu.

(2) Press the **Built-in** softkey to enter the built-in wave menu.

(3) Press **Common**, **Medical Treatment**, **Standard** softkeys to select the built-in wave type.

Press **NextPage** softkey to enter the next page, select the built-in wave type: **Maths**, **Trigonometric**, **Window function**.

Press **NextPage** softkey to enter the next page, select the built-in wave type： **Engineering**, **Seg Mod** (Segmentation Modulation) and **Fan test**.

Note: DC is a type of built-in waveform, located in the "Common" category, named "DC".

Generate the Modulated Waveform

Supported modulation types include: AM (Amplitude Modulation), FM (Frequency Modulation), PM (Phase Modulation), PWM (Pulse Width Modulation), ASK (Amplitude Shift Keying), PSK (Phase Shift Keying), FSK (Frequency Shift Keying), 3FSK (Ternary Frequency Shift Keying), 4FSK (Quadrature Frequency Shift Keying), BPSK (Biphase Phase Shift Keying), QPSK (Quadrature Phase Shift Keying), OSK (Oscillating Keying), SUM (Sum Modulation), DSBAM (Double-Sideband Amplitude Modulation) , Sweep and Brust.

Press the **Mode** function key, to select the modulation type enter the setup menu. To turn off the modulation, press the **Mode** function button again.

Parameters of modulated waveforms:

Type	Parameters	
AM	Internal source	Shape,Frequency, Depth
	External source	None
DSBAM	Internal source	Shape,Frequency, Depth
	External source	None
FM	Internal source	Shape, Frequency, Deviation
	External source	Deviation
PM	Internal source	Shape, Frequency, Deviation
	External source	Deviation
PWM	Internal source	Shape,Rate, Deviation
	External source	Deviation
ASK	Internal source	Rate, Amplitude
	External source	Amplitude
PSK	Internal source	Rate,Deviation
	External source	Deviation
FSK	Internal source	Rate, HopFreq
	External source	HopFreq
3FSK	Rate, HopFreq1, HopFreq2	
4FSK	Rate, HopFreq1, HopFreq2, HopFreq3	
BPSK	Rate, Deviation, DataSource	
QPSK	Rate,Phase1, Phase2, Phase3	
OSK	Internal source	Frequency,OSc Time
SUM	Internal source	Shape, Frequency, Depth
	External source	None
Sweep	Internal source	Linear/Log,Sweep Time, Start Freq/Center Freq, Stop Freq/Freq Span
	External source	
	Manual source	
Burst	Internal source	Burst Period,N_Cycle/Gated,Cycles/Infinite
	External source	N_Cycle/Gated,Cycles/Infinite

Generate Sweep

In the frequency sweep mode, the generator "steps" from the start frequency to the stop frequency at the sweep rate you specify. Sweep can be generated by Sine, Square, Ramp or Arbitrary waveforms.

When the output signal is Sine, Square, Ramp or Arbitrary waveform, press the front panel **Mode** key ,then press the **Sweep** to enter the sweep mode. The parameters allowed to be set are: Sweep Time, Linear/Log, Start Frequency/Center Frequency, Stop Frequency/Frequency Span, Source.

Generate Burst

Press the **Mode** function key, then press the **Burst** enter burst mode, to generate versatile waveforms in burst.Burst can last for certain times of waveform cycle (N-Cycle Burst). Bust can apply to Sine, Square, Ramp, Pulse and Arbitrary waveforms.The parameters allowed to be set are: Burst Period, Cycles/Infinite and Trigger source.

Store

Supports communication with a computer via a USB port. Using the Waveform Editor software installed on the computer, the signal generator can be operated on the computer to control the output and write of the signal generator.

The instrument settings can be saved as files in internal memory. Up to 16 instrument settings can be saved in the instrument internal memory.
Note: Please go to our official website to obtain the Waveform Edito communication software and install it.

Reading waveform

(1) Please visit our official website to obtain the installation package and decompress it.


(2) Double click " Waveform Editor " icon to run the software.



(3) Enter the “Waveform Editor” interface.

(4) Select the required waveform on the instrument.

(5) Under Waveform Editor software interface, click "Read Waveform Icon " button, and the waveform will be read and displayed on the screen.

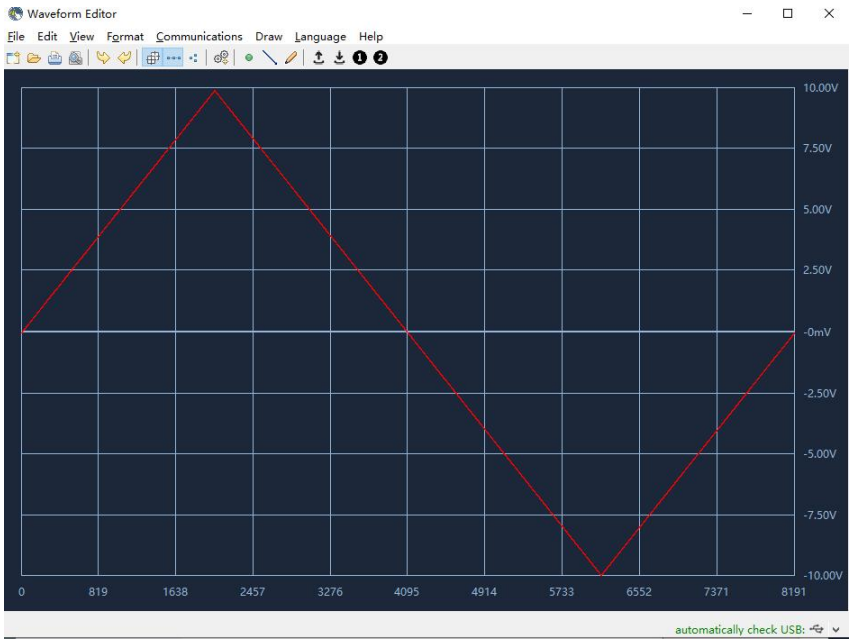

Write and Recall waveform

Users can use the Line Draw, Hand Draw and Point Edit mode in the Waveform Editor to edit the required waveform, and save and display it on the instrument by writing.

(1) Under Waveform Editor software interface, Click "Write waveform Icon " button.

(2) After the writing is successful, the "File transfer completed" prompt box will be displayed in the waveform editor, Click "Ok".

(3) On the instrument, the screen shows "Any wave has been updated to USERX(X is 0-15)".

(4) Press the button ,then press the **NextPage** button to enter the NextPage menu.

(5) Press the **Store** softkey to enter the file system, and then press the **Enter** soft key to enter the file system. Select the file name “USERX” that has just written the waveform.

(6) Press the **Call out** softkey, the screen displays "File read successfully", then press the button, the written waveform can be viewed on the

instrument.

Note: The file size is displayed on the right of the file. If 0B is displayed, the file is empty.

Utility Setting

Press the front panel **Utility** function key to enter the system options menu. The user can set the display parameters of the signal generator, CH1/2 parameters, interface parameters and system parameters. Press **Utility** again to exit the system options menu.

Utility system menu:

Menu	Description
Display Setting	
Backlight	Set the parameter value of the screen brightness.
Screen saver	Set the On/Off screen saver； If set to ON, the screen saver time range can be 1 to 999 minutes.
Separator	Set the separator for the screen display data.
CH1/2 Setting	
CH1 Load	It is convenient for the user to match the display voltage with the desired load. The range is from 1 Ω to 10 kΩ.
CH2 Load	
Sync	Enable/disable sync output terminal to output sync signal.
System Setting	
Language	Select instrument interface language.
Beeper	If On, it makes sounds when prompted.
USB Dev	Set the communication protocol type of the USB Device interface on the rear panel. **PC:** This is the internal communication protocol. Select this option when connecting to the Waveform Editor software running on computer via the USB Device interface. **USBTMC:** Select this when you need to use the USBTMC communication protocol standard.
Factory Set	Factory restoration.
Upgrade	The instrument firmware can be updated using a USB storage device through the rear panel USB interface.
Counter Setting	
HF Rejection	Enable/disable high frequency rejection.
Align Phase	Set the phase of the output signals of the two channels to be consistent.

Counter

The frequency counter measures signals in the frequency range from 100 mHz to 200 MHz. The **[Counter]** connector on the rear panel is used by default to

receive the frequency counter input signal. The frequency meter works from the start.

(1) Press the **Utility** function key ,then press the **Counter** to enter the frequency counter interface.

(2) Connect the signal to be tested to the **[Counter]** connector on the rear panel.

(3) Press the **HF Rejection** softkey to toggle On or Off high frequency rejection. High-frequency rejection can be used to filter high-frequency factors when measuring low-frequency signals, improving measurement accuracy. When measuring low frequency signals with a frequency less than 1 kHz, turn on high frequency rejection to filter out high frequency noise interference; turn off high frequency rejection when measuring high frequency signals with frequencies greater than 1 kHz.

(4) The frequency, period and duty cycle can be viewed on the frequency meter interface.

5. Communication with PC

Supports communication with a computer via a USB port. Using the Waveform Editor software installed on the computer, the signal generator can be operated on the computer to control the output and write the file to the signal generator.

The instrument settings can be saved as files in internal memory. Up to 16 instrument settings can be saved in the instrument internal memory.
Note: Please go to our official website to obtain the Waveform Editor communication software and install it.


Install communication software

(1) **Set the USB device protocol type of the signal generator**: Press **Utility** →**System** → **USB Dev**, switch to PC.

(2) **Connection:** Connect the USB Device interface on the rear panel of the signal generator to the **USB interface** of the computer with a USB cable.

(3) **Install the driver:** Run Waveform Editor software on the computer. Follow the instructions to install the driver. The path of the driver is the USBDRV folder in the directory where the Waveform Editor communication software is located, such as "C:\Program Files (x86)\DS_Wave\Waveform Editor\USBDRV".

(4) **Host computer communication port setting:** Open the Waveform Editor software,click “**Communications**” in the menu bar,select “**Ports-Settings**”, in the setting dialog box, select the communication port as “**USB**”. After the connection is successful, the connection status prompt in the lower right corner of the software interface turns green,as shown in the below figure.

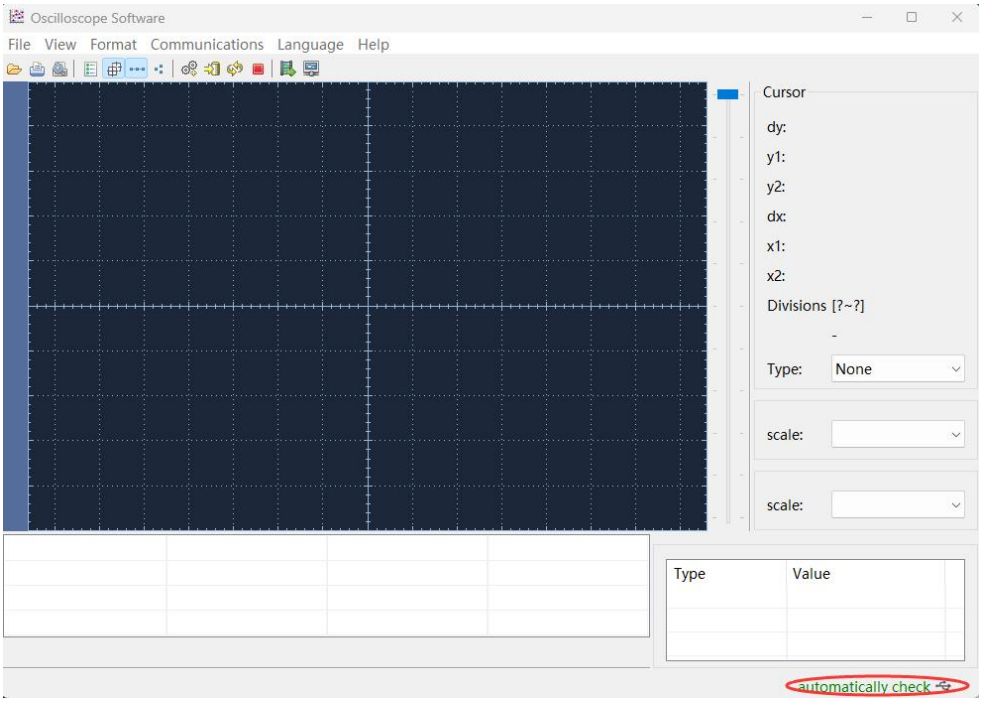

6. Appendix

Appendix A：Accessories

- 1 × power cord that meets the standards of the country where you are located
- 1 × Quick Guide
- 1 × BNC/Q9 cable
- 1 × BNC to alligator cable
- 1 × USB communication cable

Appendix B：General Care and Cleaning

General Maintenance

Do not store or leave the instrument where the liquid crystal display will be exposed to direct sunlight for long periods of time.
Caution: To avoid any damage to the instrument or probe, do not exposed it to any sprays, liquids, or solvents.
Cleaning
Inspect the instrument and probes as often as operating conditions require. To clean the instrument exterior, perform the following steps:
1. Wipe the dust from the instrument and probe surface with a soft cloth. Do not make any scuffing on the transparent LCD protection screen when clean the LCD screen.
2. Disconnect power before cleaning your instrument. Clean the instrument with a wet soft cloth not dripping water. It is recommended to scrub with soft detergent or fresh water. To avoid damage to the instrument or probe, do not use any corrosive chemical cleaning agent

⚠ **Warning:** Before power on again for operation, it is required to confirm that the instrument has already been dried completely, avoiding any electrical short circuit or bodily injury resulting form the moisture.

2024.10 V1.0.3